Drägermedical

A Dräger and Siemens Company

Field Service Procedure

GCX Suction Canister Mounting Assembly
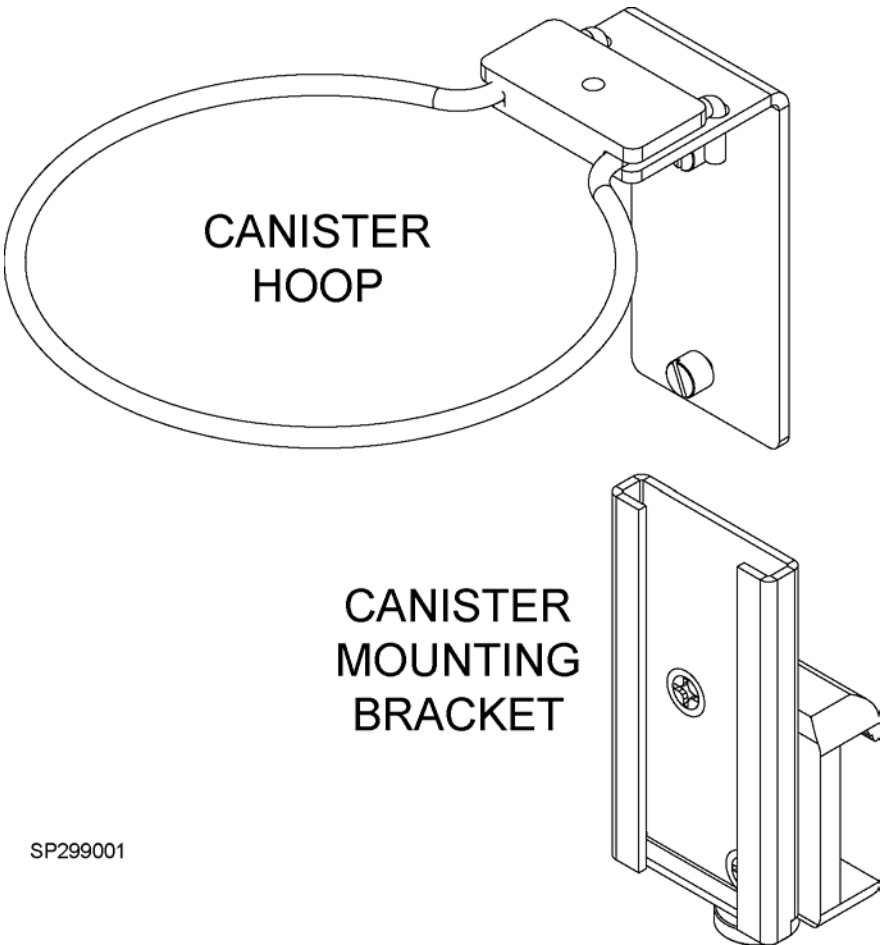## Anesthesia

Revision -
12/3/03
SP00299

GCX Suction Canister Mounting Assembly

| 1 | Purpose | The purpose of this document is to provide instruction for the mounting of the Suction Canister Mounting Assembly Kit onto a 10mm rail (not provided). |

1.1   List of Parts and Mounting Hardware

The following parts are included within this installation kit.

ITEM	QUANTITY	DESCRIPTION
1	1	Canister Mounting Bracket
2	1	Canister Hoop

SP299001

Fig. 1   GCX Suction Canister Mounting Assembly

Dräger Medical, Inc.   SP00299   Revision – Released   1
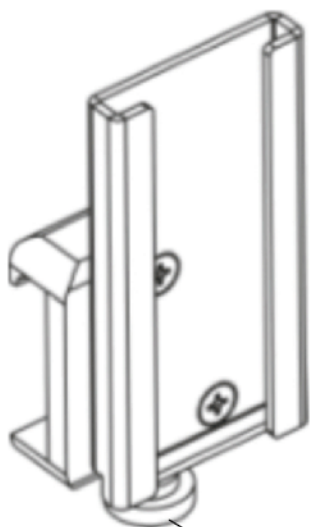
GCX Suction Canister Mtg. Assy	Service Procedure

2 Installation Procedure

2.1 Mounting the Suction Canister Bracket

1. Hook the Canister Mounting Bracket over the 10mm rail (not provided). Tighten the clamping knob (bottom of Mounting Bracket) to secure the Bracket to the rail.

CLAMPING KNOB

SP299002

Fig. 2 Mounting and Suction Canister Bracket

2. Mount the Suction Canister Holder (with mounting detail) in the channel.
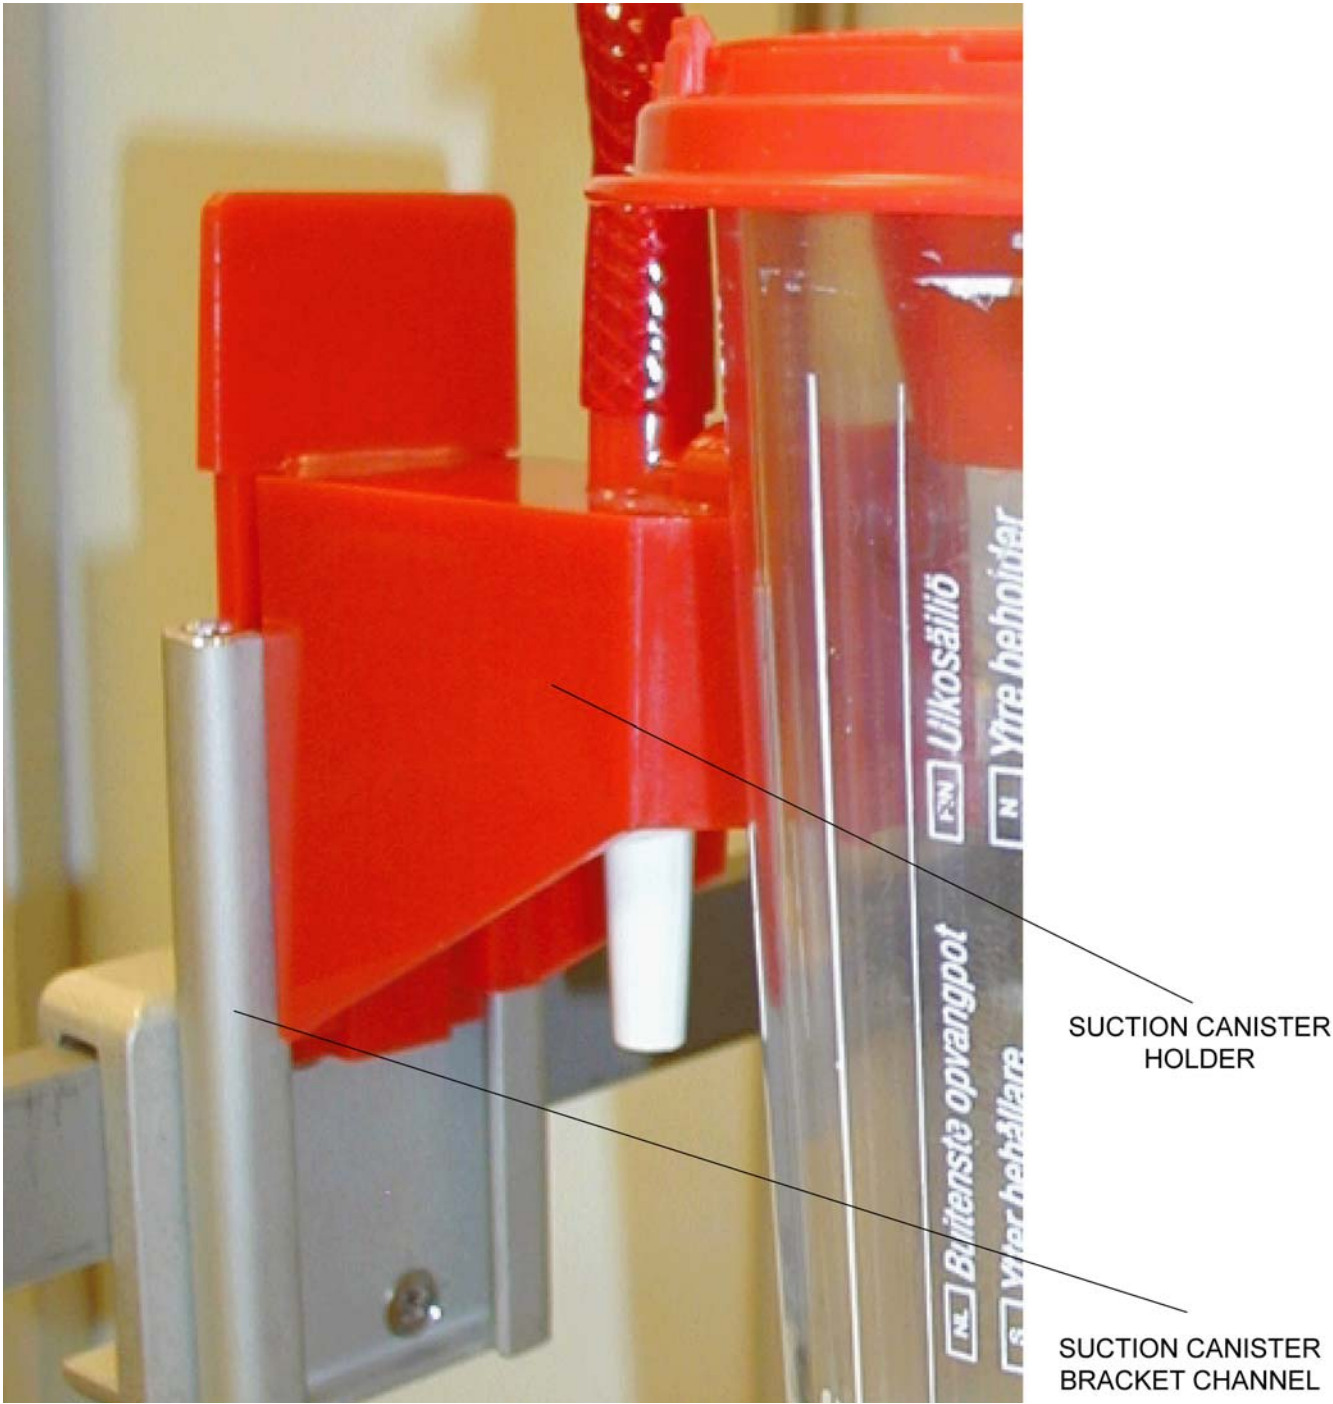
SP299.fm 11.12.03

SUCTION CANISTER
HOLDER

SUCTION CANISTER
BRACKET CHANNEL

Fig. 3   Mounting the Suction Canister to the Channel

GCX Suction Canister Mtg. Assy   **Service Procedure**

> **i**
>
> NOTE:
>
> If the Suction Canister does not provide a mounting detail, refer to Section 2.2 Mounting the Canister Hoop.

2.2 Mounting the Canister Hoop

1. Slide the Canister Hoop into the channel and tighten the two nylon screws.
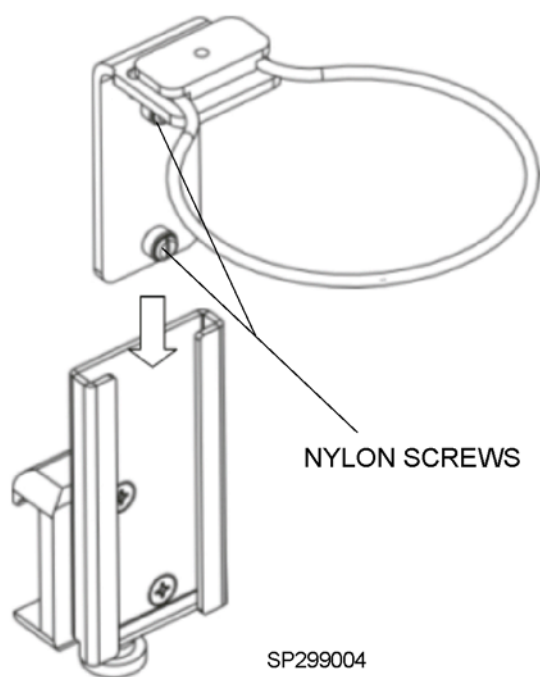
2. Insert the Suction Canister in the Canister Hoop.

Fig. 4 Mounting the Canister Hoop

SP299.fm 11.12.03

In the United States:

Draeger Medical, Inc.

3136 Quarry Road

Telford, PA 18969

USA

Tel: (215) 721-5402

   (800) 543-5047

Fax: (215) 721-5785

In all other countries:

Drëger Medical AG & Co. KGaA

Moislinger Allee 53 ć 55

D-23542 L¬beck

Germany

Tel: (++49) (0) 1805-3723437

Fax: (++49) 451/882 - 3779

GCX Suction Canister Mounting Assembly en

SP00299

Subject to change without notice.

Will not be replaced in the event of modifications.